



Labdisc™ ENVIRO

For environmental
science

LABDISC ENVIRO

+ GLOBILAB X SOFTWARE



QUICK START GUIDE

Contents

1. Labdisc Hardware Overview	3
1.1 What's in the Pack	3
1.2 Ports and Controls	3
1.3 Built-in Sensors	5
1.4 Using the Labdisc	7
1.4.1 Labdisc display.....	7
1.4.2 Labdisc keys.....	9
1.4.3 Labdisc menu	9
1.4.3.1 Setup the Labdisc for logging session	9
1.4.3.2 Labdisc information.....	10
1.4.3.3 Configuration of the Labdisc.....	11
2. Globilab X Analysis Software	12
2.1 Software Installation.....	12
2.2 Software Functions	12
2.3 Software Icons and their Functions	13
3. Labdisc – GlobiLab X Communication	20
3.1 Connect the Labdisc through a USB cable	20
3.2 Bluetooth Wireless Communication	20
3.2.1 Connect a Labdisc BLE unit	20
3.2.2 Connect Labdisc Bluetooth Classic unit	20
3.2.3 Communicating with Globilab X web version	21
5. Experiment Samples.....	25

1. Labdisc Hardware Overview

1.1 What's in the Pack

- ① Labdisc data logger
 - ② Labdisc AC charger
 - ③ USB cable
 - ④ Quick start guide
 - ⑤ Software flyer
 - ⑥ Temperature probe
 - ⑦ Colorimeter 5 cuvettes set
 - ⑧ pH electrode
 - ⑨ Dissolved oxygen electrode
- (Must be ordered separately)**




1.2 Ports and Controls

The picture below reviews the **Labdisc** ports, sensors, keypad and display:

- ① On/Off and Escape key
- ② Scroll key
- ③ Select key
- ④ Sensor selection keys
- ⑤ Graphical display 128 x 64 pixels
- ⑥ Rotating ring





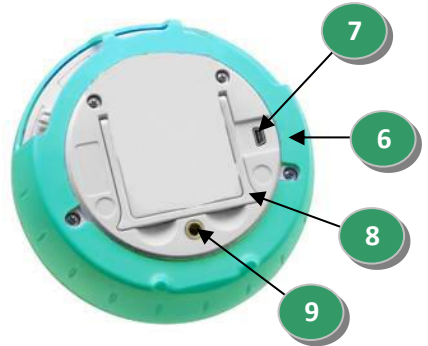








- ⑦ USB port
- ⑧ Plastic leg
- ⑨ M5 screw insert
- ⑩ Colorimeter and turbidity sensor
- ⑪ External temperature input
- ⑫ Relative humidity
- ⑬ IR temperature









- ⑭ Sound level
- ⑮ pH input and dissolved oxygen
- ⑯ Barometric pressure
- ⑰ GPS sensor
- ⑱ UV and universal input



1.3 Built-in Sensors

Icon	Type	Range	Description	Max. Sample Rate	External Accessories (supplied with Labdisc)
	Ambient temp.	-10 °C to 50 °C	Measuring ambient temperature	1/s	Not required
	Barometric pressure	500 to 1100 mB	Measuring barometric air pressure	1/s	Not required
	Colorimeter	10 - 90 % transmittance (3 colors)	Measuring solution transmittance in 3-light wavelength: Red, Green, Blue	1/s	 Cuvette set
DO ₂	Dissolved oxygen	0 to 14 mg/l	Measuring distance	10/s	 Dissolved oxygen electrode
	External temp.	-25 °C to 125 °C	General purpose stainless steel temperature probe	10/s	 Temp. probe
	GPS	N/A	Measuring 6 different parameters: Longitude, latitude, course, speed, date and time	1/s	Not required
	Infra-red temperature	-70°C to 380°C	Contactless temperature measurement. No need to touch the measured body	1/s	Not required
	pH	0 to 14 pH	Measuring pH level	10/s	 pH electrode


Icon	Type	Range	Description	Max. Sample Rate	External Accessories (supplied with Labdisc)
	Relative humidity	0 to 100% RH	Measuring relative humidity	1/s	Not required
	Sound level	56 to 95 dB	Measuring sound level	10/s	Not required
	Turbidity	0 to 1000 NTU	Measuring water turbidity level	1/s	 Cuvette set
	Ultra Violet (UV) Radiation	0 to 400 W/m ²	Measuring sun UV radiation	10/s	Not required
	Universal input	0 to 5 V	Connecting Fourier or Vernier analog sensors	100,000/s	Universal input adapter cable

1.4 Using the Labdisc

CHARGE THE LABDISC BATTERY BEFORE STARTING


Before working with the **Labdisc** for the first time, the unit should be charged for six hours with the supplied 6 V charger. The **Labdisc** charging input is located to the left of the **On/Off** key. Simply rotate the orange ring until the charging input on the **Labdisc** is exposed and then connect the charger plug to the charging input.

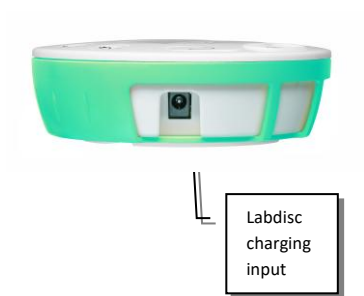

The **Labdisc** charger will accept any input voltage ranging from 100 to 240 VAC 50/60 Hz, making it functional worldwide.



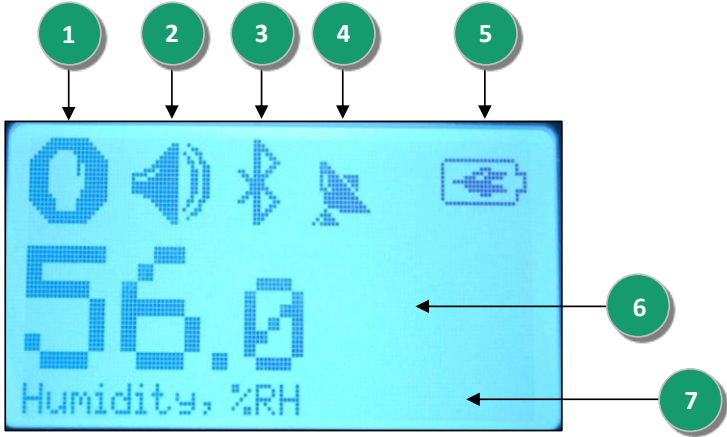



1.4.1 Labdisc display



The **Labdisc** LCD display allows users to see the different sensor readings and to setup or re-configure the Labdisc parameters.





① **Run/Stop icon** – shows  when the **Labdisc** is logging data, or  when the **Labdisc** is not logging sensor data.

② **Sound Status** – shows  active sound beep when the key is pressed and  when the sound beep is disabled.


③ **Communication Status** – shows  when Bluetooth communication is enabled, or  when the USB cable is connected from the host computer to the **Labdisc**.

④ **GPS Status** – shows  when the GPS is enabled,  when locked to GPS satellites and provides valid positioning parameters.

- ⑤ **Battery Level** – shows battery capacity at 3 levels , or  when the **Labdisc** is connected to the external charger.
- ⑥ **Sensor Value** – shows the selected sensor value.
- ⑦ **Sensor Name and Unit** - shows the selected sensor name and unit.

1.4.2 Labdisc keys


The **Labdisc** 10 keys are divided into 7 sensor keys and 3 control keys. Using the sensor keys users can select and view different sensor readings. The control keys are used to turn on/off the **Labdisc**, setup the device for the next logging session and configure all its parameters. The 3 control keys are:

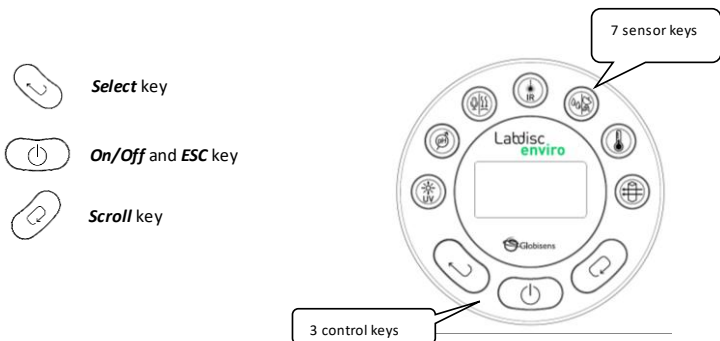


1.4.3 Labdisc menu

Press the **scroll** key to enter the Labdisc menu. Then use the **scroll** key to scan the menu options, the select key to choose a menu option and the **ESC** key to go one level up in the menu.


1.4.3.1 Setup the Labdisc for logging session

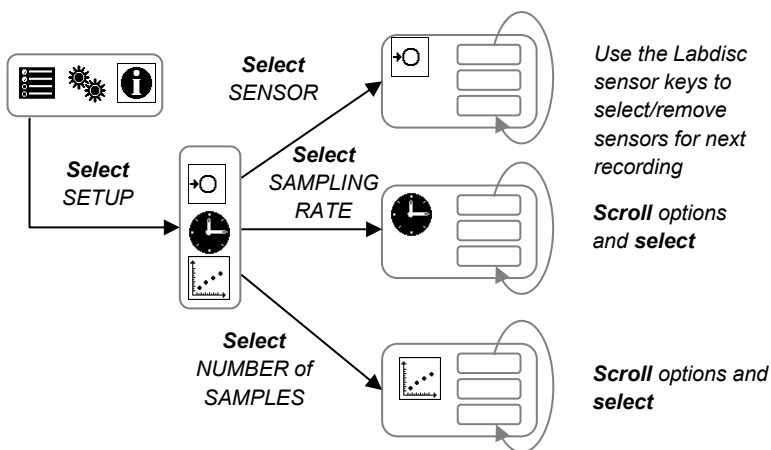

1.4.3.2 Labdisc information

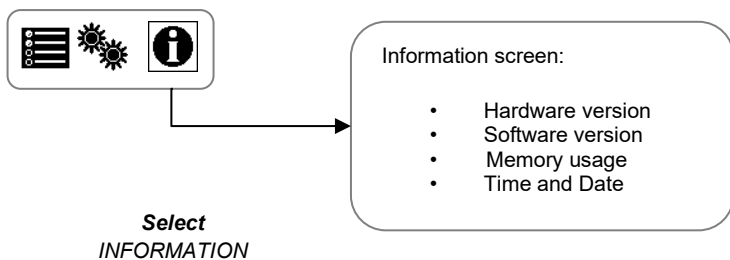

1.4.3.3 Configuration of the Labdisc

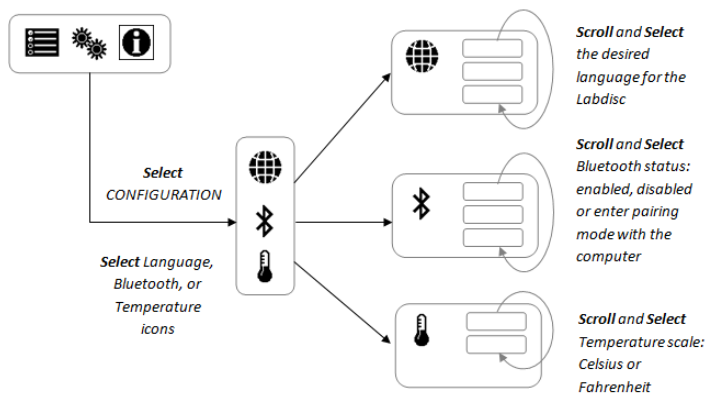

2. Globilab X Analysis Software


2.1 Software Installation

Our **GlobiLab X** software is available on Globisens website for free download. Simply go to: <https://globisens.net/support/downloads/> and choose the software version you like to download.






- For PC: GlobiLab X MSI installation for WINDOWS
- For Mac: GlobiLab X installation for MAC

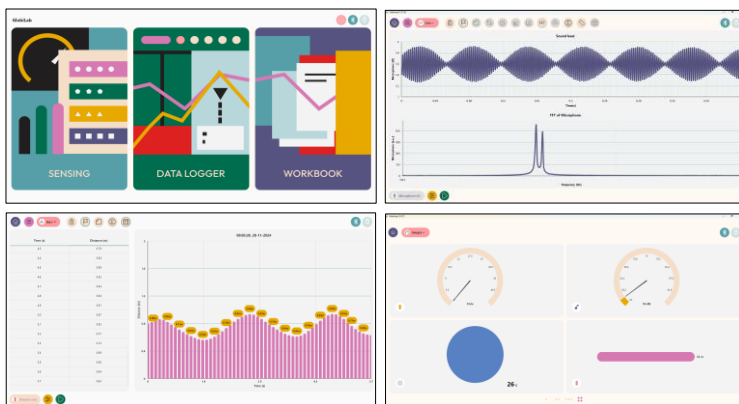













Alternatively, you may use GlobiLab X installation free web version at: www.globilab.com or the GlobiLab X iOS and Android versions in both App store and Google play store








2.2 Software Functions

















2.3 Software Icons and their Functions

	<p><i>GlobiLab X open screen – allowing users to navigate between:</i></p> <ul style="list-style-type: none">• SENSING – variety gauges display showing the current values of the Labdisc sensors.• DATA LOGGER – fully featured data collection and graphic analysis software.• WORKBOOK – a collection of experiment guides, divided into science subject: Biology, Chemistry and Physics. 
	<p><i>Communicating with the Labdisc is done either by Bluetooth or USB.</i></p> <p>USB – connect the Labdisc to the computer and click on the GlobiLab X top right USB icon. The USB icon turns green and the Labdisc is connected. </p> <p>Bluetooth - click Globilab X Bluetooth icon. A dialog box opens listing all near-by Labdisc units. Select your Labdisc, by clicking on Labdisc_XXXX, where XXXX represent the last 4 digits of your Labdisc Serial number. Bluetooth icons turns green and the Labdisc is connected. </p> <p><i>For more details on communicating with the Labdisc – please refer to chapter 3 in this manual.</i></p>

	<p>Select SENSING to view Labdisc sensors as gauges or Bar graph. Use the display type icon  to switch between Gauges and Bar Graph.</p> <p>Gauges – clicking on any of the gauges to select different sensor or different gauge type for this display. Click on the bottom  to view 1,2,3 or 4 gauges.</p> <p>Bar Graph – use the bottom left icon  to select a sensor. Then click  to view a Bar graph for this sensor.</p>
	<p>Select the DATA LOGGER to collect sensors data, view them as graphs, tables, bar graphs and even as a layer of data over Google Map.</p> <p>DATA LOGGER icons are explained below:</p>
	<p>Setting up the Labdisc is done by selecting the SETUP icon  at the bottom left of the DATA LOGGER screen. The software will open a dialog box, where you can select/remove sensors, set the sampling rate and the amount of samples for the next data recording.</p>
	<p>Click the PLAY icon  to start data collection.</p>
	<p>Click the STOP icon  ends the current data collection session.</p>
	<p>Change the Active Sensor, sensor color, or choose between sample or line graph by using the bottom right Graph Setting icon . Selecting an Active Sensor will set the Y axis for this sensor and have all graph analysis functions working on that sensor.</p>

	<p>Use Markers to get the X,Y coordinates of any point on the graph.</p> <p> Selecting the MARKER icon activates Marker mode. When in Marker mode – clicking on any point of the graph will place a graph marker. You may click and hold the Marker black point to drag it to a different graph point.</p> <p>It's possible to place up to two markers. Clicking on the Marker text box, allows you to delete it or have it pinned to a graph point.</p> <p>Click the marker icon again to leave this mode.</p>												
	<p>Use annotation to annotate the graph with texts and pictures.</p> <p> Selecting the ANNOTATION icon activates Annotation mode. When in Annotation mode – clicking on any point of the graph will place an annotation icon on the graph.</p> <p>Clicking the Annotation icon again exits the Annotation mode.</p>												
	<p>Click the CROP icon  to cut the data outside the markers area. Crop function is active only when there are 2 markers on the graph.</p>												
	<p>STATISTICS provides useful information about the graph and the active sensor. Click Statistic icon to view the Sensor type, amount of samples, sampling rate and the min, max and average for that sensor.</p> <table border="1" data-bbox="656 1196 888 1306"> <thead> <tr> <th>Sensor</th> <th>Samples</th> <th>Rate</th> </tr> </thead> <tbody> <tr> <td>Heart rate</td> <td>798</td> <td>25/Sec</td> </tr> <tr> <td>Maximum</td> <td>Minimum</td> <td>Average</td> </tr> <tr> <td>105 bpm</td> <td>75 bpm</td> <td>81 bpm</td> </tr> </tbody> </table>	Sensor	Samples	Rate	Heart rate	798	25/Sec	Maximum	Minimum	Average	105 bpm	75 bpm	81 bpm
Sensor	Samples	Rate											
Heart rate	798	25/Sec											
Maximum	Minimum	Average											
105 bpm	75 bpm	81 bpm											

	<p>Clicking any of these FUNCTIONS allows the user to apply the mathematical functions to the graph. All functions work between 2 graph markers:</p> <p> Selecting the Linear regression will display the best linear line that fits the graph between the locations of two markers. Next to the line the software will open a small text box displaying the linear line equation: $Y = aX + b$.</p> <p> Selecting the Quadratic regression will display the best parabolic line (2nd degree) that fits the graph between the locations of two markers. Next to the line the software will open a small text box displaying the parabolic line equation: $Y = aX^2 + bX + c$.</p> <p> Selecting Derivative will create a derivative graph of the active sensor data.</p> <p> Selecting the FFT will split the graphic display and show the original measurement on a time scale in the top graphic window, and its harmonics, on a frequency scale in the bottom graphic window.</p>
	<p> Selecting Average will replace the graph with an average graph. Each point in the average graph is made from an average of X samples before and X samples after this point. This function is useful in case the graph is very noisy. A dialog box will allow you to select the X (between 3 to 11)</p>
	<p> Using this TABLE icon will open a table to the left of the line graph or bar graph windows, allowing users to view simultaneously graphs and numeric data.</p>

	<p>Before running an experiment, you can add a PREDICTION line to your graph in Line Graph mode. To do so, click on this pencil icon  .</p> <ul style="list-style-type: none"> • Check/change your Y-Axis to make sure it is at a range you would expect. • Go into your Experiment Setup and choose a number of samples corresponding to the length you want for the X-Axis. <p>Then, select a point on the graph. Click a second point on the graph and a straight line will be drawn between them. As you add additional points, the line will smooth between all provided points.</p> <p>When you click play, your sensor readings will be added to the same screen so you can see your prediction and your actual data on the same graph.</p>
	<p>Clicking on the HUNBURGR icon  opens a dialog box allowing you to Save experiments, Open saved experiments and directly export all data to EXCEL. In addition, with the Add option you may open an additional saved graph, in the same graphic window – allowing you to compare two or more measurements graphs.</p>  <p>Last but not least – you may access the Labdisc 1,000,000 measurements memory, by clicking the Download from Labdisc. This opens the below dialog box – allowing you to download any of the stored recording, clear the Labdisc last recording or all recordings.</p>

Download from Labdisc



Date	Time	Rate	Samples	Sensors
18 May 2025	21:52:56	10/sec	100	
18 May 2025	21:55:03	1/sec	100	
18 May 2025	21:58:40	1/sec	100	
18 May 2025	22:00:31	1/sec	143	
18 May 2025	22:03:14	1/sec	37	
18 May 2025	22:04:06	10/sec	325	
18 May 2025	22:04:56	10/sec	44	
18 May 2025	22:07:26	1/sec	3	




Download

Clear last

Clear all

3. Labdisc – GlobiLab X Communication




3.1 Connect the Labdisc through a USB cable


- Connect the USB cable between the Labdisc rare Mini-USB socket, and your computer.
- Open the GlobiLab X software and click the most right top icon .
- The Labdisc will make a beep sound and will connect to the software.
- The USB icon   turns green indicating: successful connection with the Labdisc.




3.2 Bluetooth Wireless Communication

All Labdisc units produced in 2025 and after are using BLE (Bluetooth Low Energy) radio. Older units are using Classic Bluetooth radio. Note: the first 4 digits of every Labdisc Serial Number indicates the production year.

3.2.1 Connect a Labdisc BLE unit

- Open GlobiLab X software.
- Click the top right Bluetooth icon .
- A dialog box opens listing all near-by Labdisc.
- Select your Labdisc, by clicking the **Labdisc_XXXX**, where **XXXX** represent the last 4 digits of your Labdisc Serial number.
- The Bluetooth icons   turns green and the Labdisc is connected.



	
Labdisc_8959	
Labdisc_1026	

3.2.2 Connect Labdisc Bluetooth Classic unit

When using the **Labdisc** for the first time - it should be added as a Bluetooth device to the computer in a process called pairing. Pairing need be done only once for each **Labdisc**, after which the computer stores the connection information, including a unique name for each **Labdisc**.

Pairing steps:


- Turn on the Labdisc.
- Go to your computer Bluetooth Devices menu and click **Add a Bluetooth device**.
- The computer opens the “add a device” dialog box and starts scanning for near-by Bluetooth devices.
- Your Labdisc will be displayed as “**Labdisc-xxxx**”, where “**xxxx**” are the last four digits of the Labdisc serial number. Click on your Labdisc.
- On the Labdisc: Press and hold the Scroll key for 3 seconds.
- The Labdisc will produce a long “beep” while its screen shows “**BT pairing**”
- On your computer: enter the device pairing code: **1234** and click Next.
- Wait for the computer to finish the process and announce “**Your device is ready to use**”

Your Labdisc is now paired with your computer. From now on it can connect and communicate with the Globilab X software, using the same procedure as the BLE device (see paragraph 3.2.1)

3.2.3 Communicating with Globilab X web version

When using the Globilab X version at www.globilab.com users have to select the type of Bluetooth radio their Labdisc is using.

Selecting the radio type is done using the **CONFIGURATION** window. Click the

Configuration icon . A dialog box opens. You'll find the Bluetooth Radio at the bottom of the dialog box. Choose between **Classic** and **BLE**.

GlobiLab default is **BLE**.

4. Specifications

Data Logger specifications	
Parameter	Labdisc Enviro
Supported Platforms	Standalone, PC, Mac, iPad, Linux, Android, Chromebook, WEB
Built-in Accessible Sensors	13 sensors: Ambient Temperature, Barometer, Colorimeter, Dissolved Oxygen (electrode sold separately), External Temperature, GPS, IR Temperature, pH, Relative Humidity, Sound Level, Turbidity, Universal Input and UV
Max. Sampling Speed	100,000/s
Sampling Resolution	12-bit
Internal Data Storage	1,000,000 samples
Internal Rechargeable Battery	LiPO 3.6V
Battery Life ¹	> 200 Hours
Display	Graphical LCD 64 x 128 pixels
Keypad	Yes
Communication	USB 2.0
Wireless Communication	Bluetooth low energy V5.1
Remote Data Collection	Yes
Automatic Sensor Testing & Calibration	Yes
Size	φ=132, H=45 mm
Weight	300 gr.
Temperature Range	-10 to 50 °C
Standard Compliance	CE, FCC

¹ For sampling rate of 1 per minute



Built-in Sensor Specifications		
Sensor Type	Max. Range	Accuracy
Ambient Temperature	-10 to 50 °C	±1 °C
Barometric Pressure	500 to 1100 mB	±2.5 mB
Colorimeter	10 to 90% transmittance (3 colors) λ R=620 nm λ G=550 nm λ B=470 nm	±5 %
Dissolved Oxygen	0 to 14 mg/l	±8 %
External Temperature	-25 to 125 °C	±2 %
GPS	N/A	±3m
IR Temperature (Wide)	-70 to 380 °C	±0.5 °C @ 0 to 60°C ±1 °C @ 60 to 120°C ±1 °C @ -40 to 0°C ±2 °C @ 120 to 380°C ±2°C @ -70 to 40°C
pH	0 to 14 pH	±2 %
Relative Humidity	0 to 100 %RH	±3.5% (20% to 80%) RH
Sound Level	56 to 95 dB	±4 dB
Turbidity	0 to 1000 NTU	±10 %
UV	0 to 12 UV Index	±5 %

Analysis Software Specifications	
Parameter	Description
Data Retrieval	Online up to 100 samples per second, or download Labdisc stored data
Data Display	Line graphs, bar graphs, tables, meters, Google Maps
Communication	USB 2.0, Bluetooth 2.0
Data Logging Configuration	Sensor selection, sampling rate, sampling points
Graph Manipulation	Placing and moving up to two markers on the graphs, zoom in/out, graph cropping, graph color change, sensor legend (allowing graph show/hide and the selection of lines/icons for the graph samples)
Graph Annotation	Text and image annotations on the graph
Mathematical Functions	Derivative, linear regression, quadratic regression, FFT
Statistics	Minimum, maximum, average, standard deviation for a selected graph
Data Manipulation	Save/open of experiment data, direct export to EXCEL, display hardcopy printout
Workbook	Full suite of built-in curriculum activities
Stored Experiments	Full suite of stored experiment data
Configuration	Sensor calibration, change of sensor units
Firmware Update	Ability to update the Labdisc firmware through a USB connection
OS	PC, Mac, Linux, iPad, Android, Chromebook, WEB

5. Experiment Samples

The GLOBILab X software includes experiment samples, for teachers and students to view, analyze, modify or repeat. In this section some interesting GLOBILab recorded experiments are reviewed. To open a recorded experiment, simply click the

Hamburger icon , then Open.

	<p><u>Temperature over one week</u></p> <p>Recording temperature and humidity over one week at the school yard.</p> <ul style="list-style-type: none"> • Sensors selected: External temperature, relative humidity • Sampling rate: 1/min • Amount of samples: 10,000 • Experiment duration: one week • Communication: Offline, data downloaded at recording's end • Data Analysis: Show temperature and humidity changes on a line graph
	<p><u>Temperature changes while driving</u></p> <p>Driving in the USA, recording temperature and GPS. Viewing the changes in temperature as a layer in Google MAP.</p> <ul style="list-style-type: none"> • Sensors selected: Temperature, GPS • Sampling rate: 1/sec • Amount of samples: 10,000 • Experiment duration: 1 hour. • Communication: Download data after the experiment is over. • Data Analysis: Show temperature changes in color code icons over Google MAP



The FCC Wants You to Know:

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- a) Reorient or relocate the receiving antenna.
- b) Increase the separation between the equipment and receiver.
- c) Connect the equipment to an outlet on a circuit different from that to which the receiver is connected.
- d) Consult the dealer or an experienced radio/TV technician.

FCC Warning

Modifications not expressly approved by the manufacturer could void the user authority to operate the equipment under FCC Rules.

NOTE: THE MANUFACTURER IS NOT RESPONSIBLE FOR ANY RADIO OR TV INTERFERENCE CAUSED BY UNAUTHORIZED MODIFICATIONS TO THIS EQUIPMENT. SUCH MODIFICATIONS COULD VOID THE USER'S AUTHORITY TO OPERATE THE EQUIPMENT.

INSTRUCTIONS CONCERNING HUMAN EXPOSURE TO RADIO FREQUENCY ELECTROMAGNETIC FIELDS

A distance of at least 20cm. between the equipment and all persons should be maintained during the operation of the equipment.



Copyright ©2011 Globisens. All rights reserved. Globisens Ltd. logos and product names are registered trademarks of Globisens Ltd. No part of this document may be reproduced by any means, nor translated to any electronic medium without the written consent of Globisens. Information contained in this document is believed to be accurate and reliable, however, Globisens assumes no responsibility for its use. Specifications are subject to change without notice. www.GLOBISENS.com

GlobiLab X supports Android versions 4.0 and up.

Made for iPad. iPad is a trademark of Apple Inc., registered in the U.S. and other countries.

“Made for iPad” means that an electronic accessory has been designed to connect specifically to iPod, iPhone, or iPad, respectively, and has been certified by the developer to meet Apple performance standards. Apple is not responsible for the operation of this device or its compliance with safety and regulatory standards. Please note that the use of this accessory with iPod, iPhone, or iPad may affect wireless performance.